

Sample is added to well at left and flow is from left to right.

Positive TB Reaction (top) = Red stripes in both the T₁ (38 and 16 kDa Antigen mix)(and usually T₂) and Control (C) positions.

Positive Mycobacteria (non-TB) (middle) = Red stripe at T₂ and C positions.

Negative Reaction(bottom) = Red stripe only in C position. The C must always be positive or the test is invalid.

2006101300T

Fig. 2

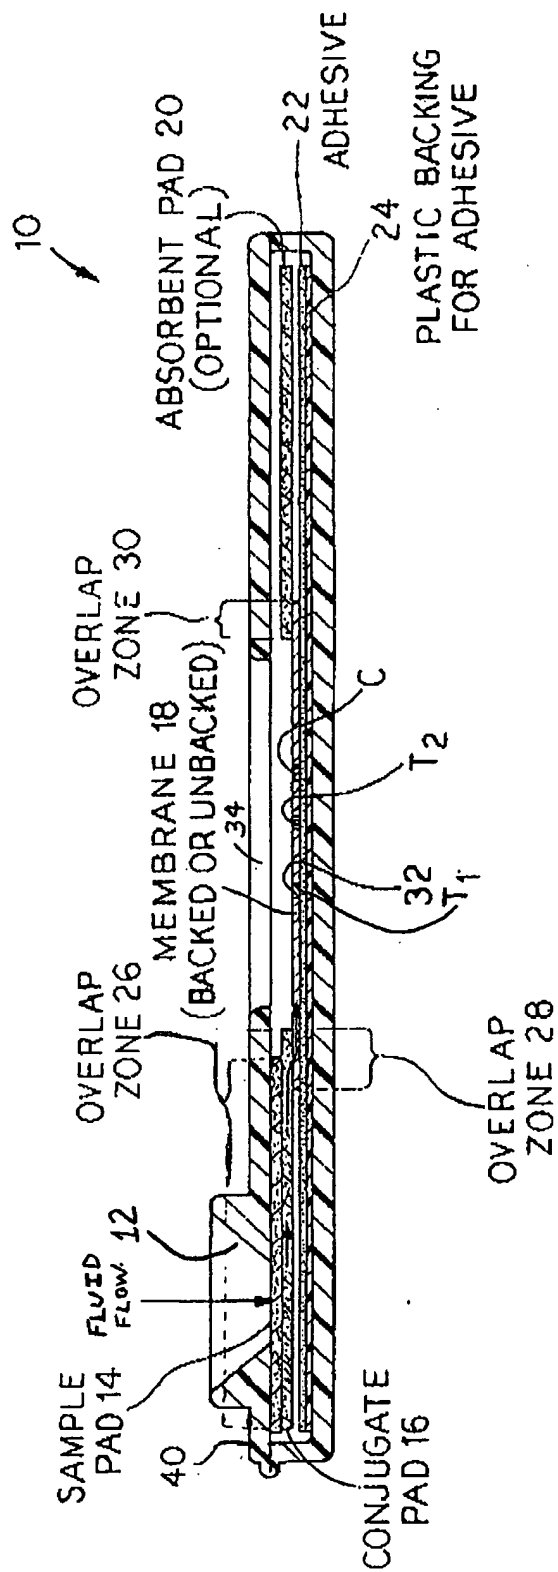


Fig.3

